

BRADY L-2588-19A UHF LAB LABEL

TDS No. L-2588-19A
Effective Date: 25/11/2020

Description:

UHF RFID Label for use on general laboratory identification on conical, bottles, test tubes, large tubes and well plate.

Details:

Material Specifications:

Face Material	B-7425 - Polypropylene
Adhesive	Permanent acrylic adhesive
Finishing	Matte
Antenna	Aluminium
IC to antenna construction	Chip bonded to antenna using Anisotropic Conductive Film adhesive
Tag base material	PET

General Specifications:

Applications	Pharmaceutical and healthcare. The RFID label is designed for used on conical, bottles, test tubes, large tubes and well plate in the laboratory environment.
Print Technology	Thermal transfer print, including RFID encoding.
Recommended Ribbon	Brady Series R7961
Operating Temperature	-40 °C to 85 °C
Regulatory/Agency Approvals	For information on the Weee-RoHS compliance status for a Brady Product go to one of the following websites: In Canada: www.bradycanada.ca/weee-rohs In Europe: www.bradyeurope.com/rohs In Japan: www.brady.co.jp/products/labelsuse/rohs All other regions: www.bradyid.com/weee-rohs

Electronic Specifications:


IC / Chip	NXP U7XM2
Operating Frequency	860 - 960 MHz (ETSI band)
Supported Standard	ISO 18000-6C, EPC Class 1, Gen 2v2
EPC Memory	448 bits
User Memory	2048 bits
TID (locked) Memory	96 bits
Reserved Memory	32 bits (for kill access passwords)

Read Range:

Details RFID performance in ETSI lower bandwidth:

PERFORMANCE PROPERTIES	TEST METHOD	TYPICAL RESULTS
RFID Read range on free air	CISC Tagformance test	up to 2.5m
RFID Read range on glass panel	CISC Tagformance test	up to 5.5m
RFID Read range on glass bottles and vials	CISC Tagformance test	up to 2.2m
RFID Read range on PP panel	CISC Tagformance test	up to 6.1m
RFID Read range on PP bottles and vials	CISC Tagformance test	up to 5.5m
RFID Read range on glass test tubes	CISC Tagformance test	up to 3.8m
RFID Read range on PP test tubes	CISC Tagformance test	up to 6.1m

Notes: There can be some variation in the read ranges in the presence of liquid. It is recommended to place the label on the area of a product with least interference with liquid. It remains the responsibility of the user to assess the risk of using this product. We encourage customers to develop testing protocols that will qualify a product's fitness for use in their actual application.

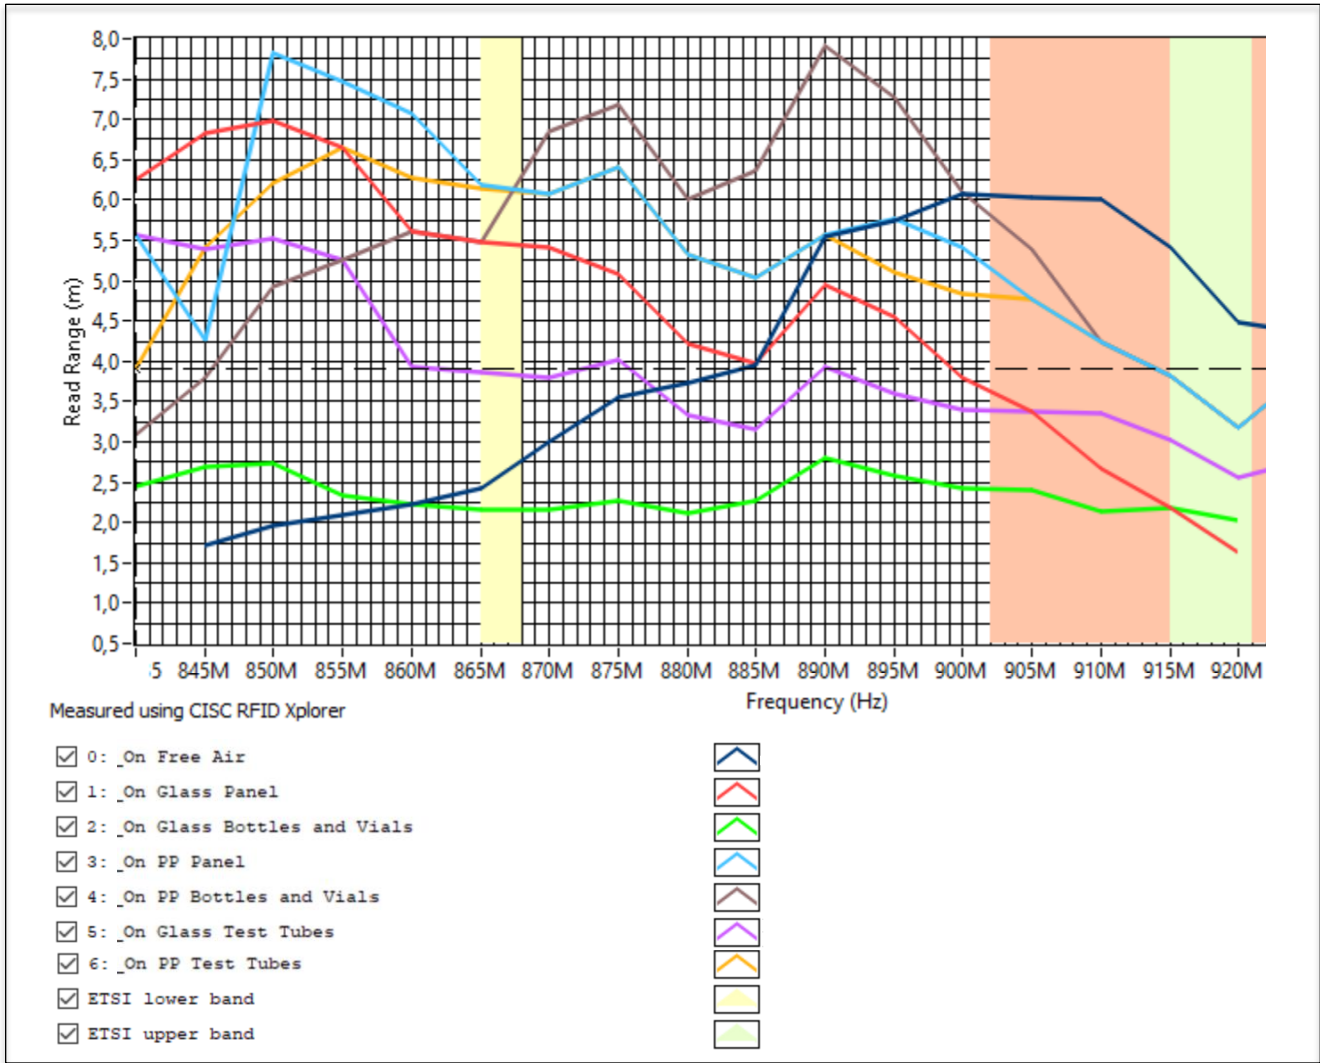


Label Dimensions:

Metric (mm)		
Width	Length	Thickness Total (with chip)
45.00	30.00	0.28

Label Mass (including antenna and chip)

Label Mass (g)
0.16

Dimensions (mm)

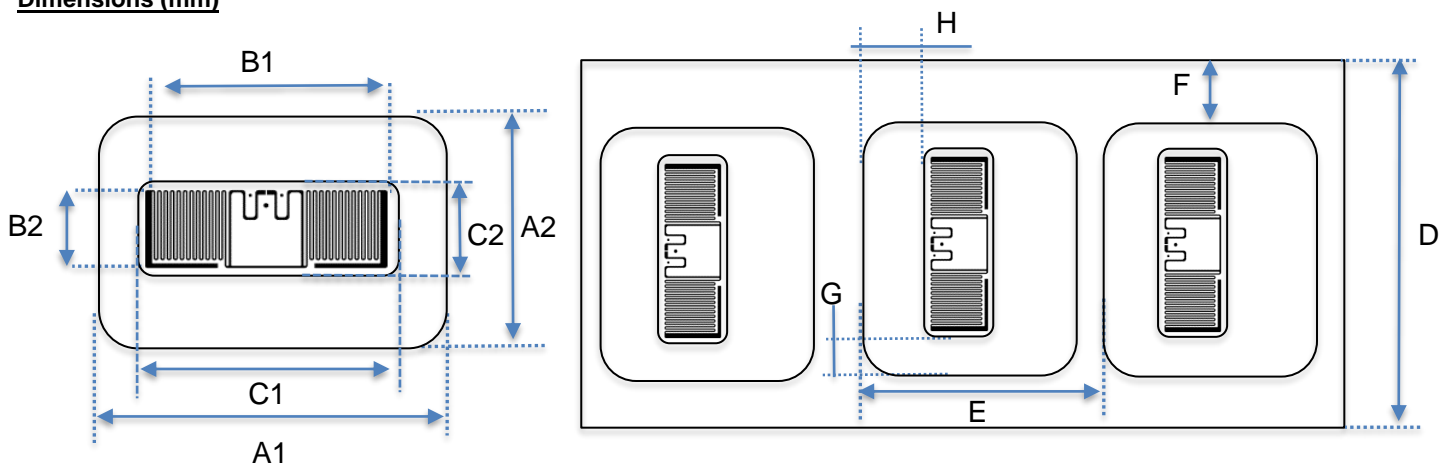

		Length (mm)	Tolerance (mm)
A1	Tag Width	45.00	+/- 0.2
A2	Tag Length	30.00	+/- 0.2
B1	Antenna Width	30.00	+/- 0.5
B2	Antenna Length	10.00	+/- 0.5
C1	Die-Cut Width	32.00	+/- 0.2
C2	Die-Cut Length	14.00	+/- 0.2
D	Web Width	55.00	+/- 0.3
E	Tag to Tag Pitch	33.00	+/- 1.5
F	Web edge to label	5.00	+/- 0.3
G	Die-Cut to side label	6.50	+/- 1.5
H	Die-Cut to top label	5.00	+/- 1.5

Delivery and Packaging Specifications

RFID labels per roll	500
Rolls in package	1
Winding	RFID labels out
Inspection and delivered tags	100% inspected, 500 good RFID labels per roll
Bad Tags Marked	Yes

Label Performance

Details:

PHYSICAL PROPERTIES	TEST METHODS	AVERAGE RESULTS
Thickness	ASTM D 1000 -Total (excluding liner)	0.011 inch (0.28 mm)
Adhesion to: -Glass	ASTM D 1000 20 minute dwell 24 hour dwell	42 N/100mm (38 oz/inch) 48 N/100mm (44 oz/inch)
-Polypropylene	20 minute dwell 24 hour dwell	33 N/100mm (30 oz/inch) 47 N/100mm (43 oz/inch)

ENVIRONMENTAL PERFORMANCE PROPERTIES		LABEL APPLIED TO ROOM TEMPERATURE SURFACE		
Samples were printed with the Brady Series R7961 thermal transfer ribbons. Samples were adhered at room temperature to the surfaces listed below.				
ENVIRONMENT	TEST METHODS	EFFECT TO LABEL ADHESION	EFFECT TO PRINT IMAGE	EFFECT TO CHIP
High Service Temperature	5 days at 70°C (158°F)	<ul style="list-style-type: none"> ✓ Glass test tube (10 mm Ø) DURAN® ✓ Glass test tube (16 mm Ø) AR® ✓ 4,5 ml PP cryovial ✓ Glass panel ✓ PP panel ✓ 20 ml glass vial (wheathon) 	No visible effect	Readable
Low Service Temperature	5 days at -80°C (-112°F)	<ul style="list-style-type: none"> ✓ Glass test tube (10 mm Ø) DURAN® ✓ Glass test tube (16 mm Ø) AR® ✓ 4,5 ml PP cryovial ✓ Glass panel ✓ PP panel ✓ 20 ml glass vial (wheathon) 	No visible effect	Readable
Simulated Incubator	3 cycles of 1 hour at 70°C (158°F) and 3 hours at room temperature	<ul style="list-style-type: none"> ✓ Glass test tube (10 mm Ø) DURAN® ✓ Glass test tube (16 mm Ø) AR® ✓ 4,5 ml PP cryovial ✓ Glass panel ✓ PP panel ✓ 20 ml glass vial (wheathon) 	No visible effect	Readable
Autoclave	5 cycles at 120°C (248°F) for 20 minutes	<ul style="list-style-type: none"> ✓ Glass test tube (10 mm Ø) DURAN® ✓ Glass test tube (16 mm Ø) AR® ✓ 4,5 ml PP cryovial 	No visible effect	Readable

		<ul style="list-style-type: none"> ✓ Glass panel ✓ 20 ml glass vial (wheathon) 		
Freezer	5 cycles of 16 hours of 16 hours at -80°C (-112°F) and 8 hours at room temperature	<ul style="list-style-type: none"> ✓ Glass test tube (10 mm Ø) DURAN® ✓ Glass test tube (16 mm Ø) AR® ✓ 4,5 ml PP cryovial ✓ Glass panel ✓ 50 ml PP tube (Falcon) ✓ PP panel ✓ 20 ml glass vial (wheathon) 	No visible effect	Readable
Liquid Nitrogen	5 cycles of 4 hours at -196°C (-320°F) and 20 hours at room temperature	<ul style="list-style-type: none"> ✓ Glass test tube (10 mm Ø) DURAN® ✓ Glass test tube (16 mm Ø) AR® ✓ 4,5 ml PP cryovial ✓ 20 ml glass vial (wheathon) 	No visible effect	Readable
Freezer to Boiling Water	1 hour at -80°C (-112°F) then placed in boiling water (100°C/212°F) for 10 minutes	<ul style="list-style-type: none"> ✗ Glass test tube (10 mm Ø) DURAN® ✗ Glass test tube (16 mm Ø) AR® ✓ 4,5 ml PP cryovial ✓ Glass panel ✓ 50ml PP tube (Falcon) 	No visible effect	Readable
Liquid Nitrogen to Boiling Water	1 hour at -196°C (-320°F) then placed in boiling water (100°C/212°F) for 10 minutes	<ul style="list-style-type: none"> ✗ Glass test tube (10 mm Ø) DURAN® ✗ Glass test tube (16 mm Ø) AR® ✓ 4,5 ml PP cryovial ✓ 50ml PP tube (Falcon) 	No visible effect	Readable

✓ = Label suitable for application; no visible effect, label remains adhered to test surface

◆ = Label may work in application; test results were mixed

✗ = Label does not work in the application

PERFORMANCE PROPERTIES		CHEMICAL RESISTANCE		
The chemical resistance of samples printed with the Brady Series R7961 black ribbons was tested at room temperature. The samples were immersed in the test solvent for 15 minutes. The samples were removed and rubbed 10 times with a cotton swab saturated with the test fluid. The samples were rated for the amount of print removal using the rating scale below.				
CHEMICAL REAGENT	EFFECT TO PRINT/TOPCOAT WITHOUT RUB	EFFECT TO PRINT/TOPCOAT WITH RUB	EFFECT TO ADHESIVE	EFFECT TO CHIPS
Ethanol	1	5	1	Readable
Toluene	1	3	1	Readable
Isopropyl Alcohol	1	3	1	Readable
Hydrochloric Acid 37%	2	5	1	Readable
Sodium Hydroxide 10%	1	5	1	Readable
Acetone	1	3	1	Readable
Xylene	1	3	1	Readable

Rating Scale

1 = no visible effect

2 = slight smear or print removal, detectable but minimal smear

3 = moderate smear or print removal (print still legible)

4 = severe smear or print removal (print illegible or just barely legible)

5 = complete print and/or topcoat removal

NP= print removed prior to rub

Shelf Life:

Shelf life is two years from the date of receipt for this product as long as this product is stored in its original packaging in an environment below 80° F (27° C) and 60% RH. It remains the responsibility of the user to assess the risk of using this product. We encourage customers to develop testing protocols that will qualify a product's fitness for use in their actual application.

Trademarks:

ANSI: American National Standards Institute (U.S.A.)

ASTM: American Society for Testing and Materials (U.S.A.)

All S.I. Units (metric) are mathematically derived from the U.S. Conventional Units.

Note: All values shown are averages and should not be used for specification purposes.

Test data and test results contained in this document are for general information only and shall not be relied upon by Brady customers for designs and specifications, or be relied on as meeting specified performance criteria. Customers desiring to develop specifications or performance criteria for specific product applications should contact Brady for further information.

Product compliance information is based upon information provided by suppliers of the raw materials used by Brady to manufacture this product or based on results of testing using recognized analytical methods performed by a third party, independent laboratory. As such, Brady makes no independent representations or warranties, express or implied, and assumes no liability in connection with the use of this information.

WARRANTY

Brady products are sold with the understanding that the buyers will test them in actual use and determine for themselves their adaptability to their intended uses. Brady warrants to the buyers that its products are free from defects in material and workmanship, but limits its obligation under this warranty to replacement of the product shown to Brady's satisfaction to have been defective at the time Brady sold it. This warranty does not extend to any persons obtaining the product from the buyers. This warranty is in lieu of any other warranty, express or implied, including, but not limited to, any implied warranty of merchantability or fitness for a particular purpose, and of any other obligations or liability on Brady's part. Under no circumstances will Brady be liable for any loss, damage, expense, or consequential damages of any kind arising in connection with the use, or inability to use, Brady's products.

Copyright 2020 Brady Worldwide, Inc. | All Rights Reserved
Material may not be reproduced or distributed in any form without written permission

Brady EMEA | Lindestraat 20 | 9240 Zele | Belgium | Tel: +32 (0) 52 45 78 11 | Fax: +32 (0) 52 45 78 12